

Quick Guide for Dario LC° Blood Glucose Monitoring System Welcome to Dario°!

PLEASE READ THESE INSTRUCTIONS BEFORE OPERATING THE SYSTEM.

PLEASE REFER TO DARIO LC' BLOOD GLUCOSE MONITORING SYSTEM USER GUIDE FOR COMPLETE INSTRUCTIONS.



6173-05 RevA

DARIC

Dario LC^{*} is an all-in-one glucose monitoring system that includes a lancing device, a strip cartridge and a miniature glucose meter in a durable shell. The miniature glucose meter connects to a compatible smart mobile device for managing your diabetes using the Dario^{*} App.

Indication for Use

The Dario LC^{*} Blood Glucose Monitoring System consists of the Dario LC^{*} Blood Glucose Meter, Dario Glucose Test Strips, Dario Glucose Control Solutions and the Dario App as the display component of the Dario LC^{*} Blood Glucose Monitoring System. The Dario LC^{*} Blood Glucose Monitoring System is intended for the quantitative measurement of glucose (sugar) in fresh capillary whole blood samples drawn from the fingertips. The Dario LC^{*} Blood Glucose Monitoring System is intended to be used by a single person and should not be shared.

The Dario LC^{*} Blood Glucose Monitoring System is intended for self-testing outside the body (in vitro diagnostic use) by people with diabetes at home to monitor the effectiveness of diabetes control. The Dario LC^{*} Blood Glucose Monitoring System should not be used for the diagnosis of or screening of diabetes or for neonatal use.

The Dario^{*} Blood Glucose Test Strips are for use with the Dario LC^{*} Blood Glucose Meter to quantitatively measure glucose (sugar) in fresh capillary whole blood samples drawn from the fingertip.

The Dario^{*} Glucose Control Solutions are for use with the Dario LC^{*} Blood Glucose Meter and the Dario^{*} Blood Glucose Test Strips to check that the meter and test strips are working together properly and that the test is performing correctly.

Upon receiving the Dario LC° Welcome Kit, verify that it includes:



- Dario LC^{*} System which includes the Lancing Device and Built-In Blood Glucose Meter with Lightning connector.
- Dario[®] 10 Sterile Lancets
- Quick Guide for Dario LC[®] Blood Glucose Monitoring System
- 10 Disposable Covers (4.37"X8.19")
- User Guide for Dario LC[®] Blood Glucose Monitoring System
- Dario[®] Test Strips (sold separately)
- Dario[®] Control Solution Level 1 and 2 (sold separately)

If anything is missing or damaged do not use the product.



Contact customer service at

1-800-895-5921, a toll-free number in the U.S., 9:00 AM - 5:00 PM EST Monday through Friday or: www.mydario.com/Support

Please contact your healthcare professional for questions outside of the customer support hours.


- ⚠️ Your Dario LC[®] Blood Glucose Meter must be used with Dario Test Strips.
- A The meter and lancing device are for single patient use. Do not share them with anyone including other family members! Do not use on multiple patients.
- All parts of the kit are considered biohazardous and can potentially transmit infectious diseases, even after you have performed cleaning and disinfection.
- ⚠️ For cleaning and disinfection please refer to Dario LC[®] BGMS user guide.

Assemble Dario LC°




Dario LC^{*} is comprised of three parts contained in one housing: a Test Strip Cartridge, a Lancing Device, and a Glucose Meter.



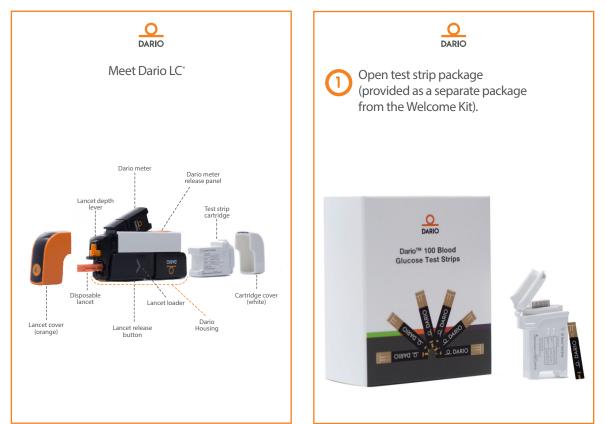



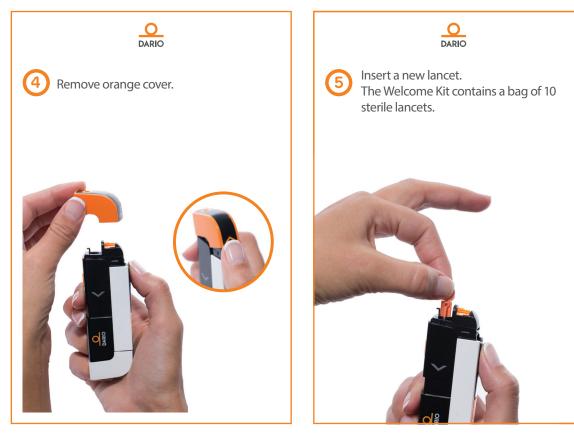








You may adjust the lancet depth to one of four settings. 1 is the shallowest and 4 is the deepest setting.







Measure with Dario LC°

O DARIO

- Insert the phone into the disposable cover included in the Welcome Kit. Place the Dario LC[°] meter port to fit the opening at the bottom of the disposable cover.
- ▲ To avoid the risk of transmitting blood borne pathogens, it is advised to use a disposable sleeve to cover your smart mobile device while taking the blood glucose test.



Open the Dario[®] application.

[9



DARIO



Slide your thumb back on the ridged orange panel to release the Dario LC° meter.





Grasp the meter with two fingers and remove it from the housing.









Plug the Dario LC° meter into the Lightning connector port. The Dario° logo should be facing up.

> Note the Dario LC° meter direction (logo facing up)

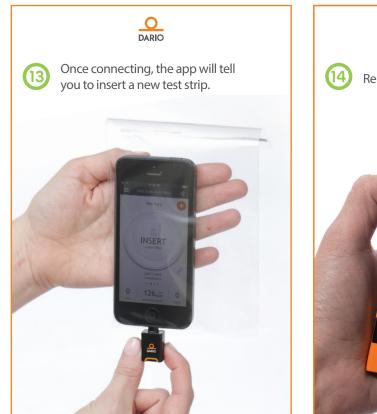



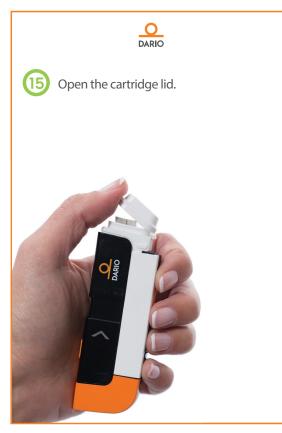



Remove a test strip. Now close the cartridge lid to protect the remaining test strips and put the white cover back on.





Insert a test strip into the test strip port. Verify the test strip direction as shown below. The app will let you know when a test strip has been successfully inserted.

126.

Test strips should not be exposed in the open air for more than three minutes.





Load the lancing device by sliding down as shown below.





Place the lancing device on to the side of your fingertip and press the lancet release button to prick your finger.







Apply a drop of blood to the tip of the test strip.





 \land







Dispose of used lancet and test strips in accordance with the instructions provided by your health care provider for biohazardous waste.







Place the Dario LC[®] meter back into the housing by pushing it in until it is locked into place.



SMART MOBILE DEVICE COMPATIBILITY:

Dario LC° is compatible for use on iOS smart mobile devices. For full list of compatible devices please refer to www.mydario.com/support/getting-started

STORAGE & SPECIFICATION:

Dario LC® Blood Glucose Monitoring System Specifications:		
Result Range	20-600 mg/dL	
Blood Source	Fresh capillary whole blood	
Calibration	Plasma equivalent	
Sample Size	0.3 microliter	
Test Time	6 seconds	
Assay Method	Glucose Oxidase Biosensor	
Power Supply	Meter receives power from the smart mobile device	
Glucose Units	mg/dL	
Display	Dario [®] application on a smart mobile device screen	
System Environmental Information		
Operating Conditions	50°F-95°F (10°C-35°C) 15-85% Relative Humidity	

	Humidity
Test Strips Storage Conditions	36°F-90°F (2°C-32°C) 10-90% Relative Humidity
Welcome kit Storage Temperature	34°F-95°F (1°C-35°C)
Operational Altitude	Up to 10.000 feet (3,048 meters)

EXPLANATION OF SYMBOLS: The following symbols may appear on the device, instructions for use, accessories or shipping materials:

O DARIO	Dario [*] logo
LS	LabStyle Innovation [®] logo
i	Consult instructions for use
IVD	In Vitro Diagnostic
LOT	Batch Code
8	Expiry date
8	Do not reuse
35°C 95°F 34°F	Temperature limitation
REF	Catalogue number

	Manufacturer: LabStyle Innovation" Ltd. 8 Hatokhen St. North Industrial Park Caesarea 3088900 Israel
Σ Σ	Contains <10> Lancets
×	Keep away from sunlight
STERILE R	Sterilized using - Gamma Irradiation
SELF	Intended for self-testing
	Do not use if seal is broken or missing.
	Warning Sign



Thriving with Diabetes

Customer support: 1-800-895-5921 toll-free number in the U.S. 9:00 AM - 5:00 PM EST Monday through Friday or: www.mydario.com/Support